

HIS (Histamine) ELISA Kit, Universal

 Cat# E0065
 store at 2-8°C

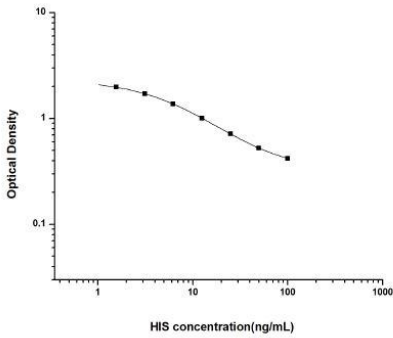
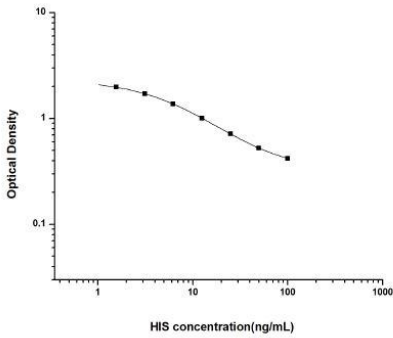
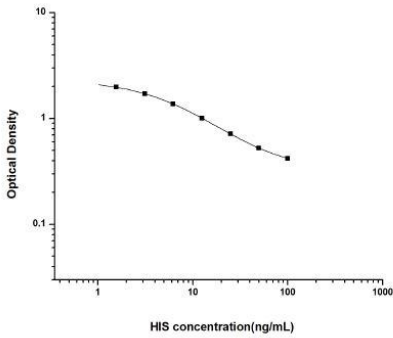
INFORMATION

Size	96T
Intended use	This ELISA kit applies to the in vitro quantitative determination of HIS concentrations in serum, plasma and other biological fluids.
Sensitivity	0.94 ng/mL
Detection Range	1.56-100 ng/mL
Specificity	This kit recognizes HIS in samples. No significant cross-reactivity or interference between HIS and analogues was observed.
Repeatability	Coefficient of variation is < 10%
Test principle	This ELISA kit uses the Competitive-ELISA principle. The micro ELISA plate provided in this kit has been pre-coated with HIS. During the reaction, HIS in samples or Standard competes with a fixed amount of HIS on the solid phase supporter for sites on the Biotinylated Detection Ab specific to HIS. Excess conjugate and unbound sample or standard are washed from the plate, and Avidin conjugated to Horseradish Peroxidase (HRP) are added to each microplate well and incubated. Then a TMB substrate solution is added to each well. The enzyme-substrate reaction is terminated by the addition of stop solution and the color change is measured spectrophotometrically at a wavelength of 450±2 nm. The concentration of HIS in the samples is then determined by comparing the OD of the samples to the standard curve.
Other supplies required	Microplate reader with 450 nm wavelength filter High-precision transfer pipette, EP tubes and disposable pipette tips Incubator capable of maintaining 37°C Deionized or distilled water Absorbent paper Loading slot
Note	<p>✓ Note for kit</p> <p>1) For research use only. Not for use in diagnostic procedures.</p> <p>2) Please wear lab coats, eye protection and latex gloves for protection. Please perform the experiment following the national security protocols of biological laboratories, especially when detecting blood samples or other bodily fluids.</p> <p>3) A freshly opened ELISA plate may appear a water-like substance, which is normal and will not have any impact on the experimental results. Return the unused wells to the foil pouch and store according to the conditions suggested in the above table.</p> <p>4) Do not reuse the reconstituted standard, biotinylated detection Ab working solution, concentrated HRP conjugate</p>

	<p>working solution. The unspent undiluted concentrated biotinylated detection Ab (100×) and other stock solutions should be stored according to the storage conditions in the above table.</p> <p>5) The microplate reader should be able to be installed with a filter that can detect the wave length at 450 ± 10 nm. The optical density should be within 0-3.5. Follow the Instructions of the Microplate Reader for set-up and preheat it for 15 min before OD measurement.</p> <p>6) Do not mix or substitute reagents with those from other lots or sources.</p> <p>7) Change pipette tips in between adding of each standard level, between sample adding and between reagent adding. Also, use separate reservoirs for each reagent.</p> <p>8) The kit should not be used beyond the expiration date on the kit label.</p> <p>✓ Note for sample</p> <p>1) Tubes for blood collection should be disposable and be non-endotoxin. Samples with high hemolysis or much lipid are not suitable for ELISA assay.</p> <p>2) Samples should be assayed within 7 days when stored at $2-8^{\circ}\text{C}$, otherwise samples must be divided up and stored at -20°C (≤ 1 month) or -80°C (≤ 3 months). Avoid repeated freeze-thaw cycles. Prior to assay, the frozen samples should be slowly thawed and centrifuged to remove precipitates.</p> <p>3) Please predict the concentration before assaying. If the sample concentration is not within the range of the standard curve, users must determine the optimal sample dilutions for their particular experiments.</p> <p>4) If the sample type is not included in the manual, a preliminary experiment is suggested to verify the validity.</p> <p>5) If a lysis buffer is used to prepare tissue homogenates or cell lysates, there is a possibility of causing a deviation due to the introduced chemical substance.</p> <p>6) Some recombinant protein may not be detected due to a mismatching with the coated antibody or detection antibody.</p>
Dilution Method	<p>Please predict the concentration range of the sample in advance. If your test sample needs dilution, please refer to the dilution method as follows:</p> <p>For 100 fold dilution: One-step dilution. Add 5 μL sample to 495 μL sample diluent to yield 100 fold dilution.</p> <p>For 1000 fold dilution: Two-step dilution. Add 5 μL sample to 95 μL sample diluent to yield 20 fold dilution, then add 5 μL 20 fold diluted sample to 245 μL sample diluent, after this, the neat sample has been diluted at 1000 fold successfully.</p> <p>For 100000 fold dilution: Three-step dilution. Add 5 μL sample to 195 μL sample diluent to yield 40 fold dilution, then add 5 μL 40 fold diluted sample to 245 μL sample diluent to yield 50 fold dilution, and finally add 5 μL 2000 fold diluted sample to 245 μL sample diluent, after this, the neat sample has been diluted at 100000 fold successfully.</p>

Reagent preparation	<p>1. Bring all reagents to room temperature (18-25°C) before use. If the kit will not be used up in one assay, please only take out the necessary strips and reagents for present experiment, and store the remaining strips and reagents at required condition.</p> <p>2. Wash Buffer: Dilute 30 mL of Concentrated Wash Buffer with 720 mL of deionized or distilled water to prepare 750 mL of Wash Buffer. Note: if crystals have formed in the concentrate, warm it in a 40°C water bath and mix it gently until the crystals have completely dissolved.</p> <p>3. Standard working solution: Centrifuge the standard at 10,000×g for 1 min. Add 1.0 mL of Reference Standard & Sample Diluent, let it stand for 10 min and invert it gently several times. After it dissolves fully, mix it thoroughly with a pipette. This reconstitution produces a working solution of 100 ng/mL (or add 1 mL of Reference Standard & Sample Diluent, let it stand for 1-2 min and then mix it thoroughly with a vortex meter of low speed. Bubbles generated during vortex could be removed by centrifuging at a relatively low speed). Then make serial dilutions as needed. The recommended dilution gradient is as follows: 100, 50, 25, 12.5, 6.25, 3.13, 1.56, 0 ng/mL. Dilution method: Take 7 EP tubes, add 500 µL of Reference Standard & Sample Diluent to each tube. Pipette 500 µL of the 100 ng/mL working solution to the first tube and mix up to produce a 50 ng/mL working solution. Pipette 500 µL of the solution from the former tube into the latter one according to this step. The illustration below is for reference.</p> <p>4. Biotinylated Detection Ab working solution: Calculate the required amount before the experiment (50 µL/well). In preparation, slightly more than calculated should be prepared. Centrifuge the Concentrated Biotinylated Detection Ab at 800×g for 1 min, then dilute the 100× Concentrated Biotinylated Detection Ab to 1× working solution with Biotinylated Detection Ab Diluent (Concentrated Biotinylated Detection Ab: Biotinylated Detection Ab Diluent = 1: 99).</p> <p>5. Concentrated HRP Conjugate working solution: Calculate the required amount before the experiment (100 µL/well). In preparation, slightly more than calculated should be prepared. Centrifuge the Concentrated HRP Conjugate at 800×g for 1 min, then dilute the 100× Concentrated HRP Conjugate to 1× working solution with HRP Conjugate Diluent (Concentrated HRP Conjugate: HRP Conjugate Diluent = 1: 99).</p>
Assay procedure	<p>1. Determine wells for diluted standard, blank and sample. Add 50 µL each dilution of standard, blank and sample into the appropriate wells (It is recommended that all samples and standards be assayed in duplicate). Immediately add 50 µL of Biotinylated Detection Ab working solution to each well. Cover the plate with the sealer provided in the kit. Incubate for 45 min at 37°C. Note: solutions should be added to the bottom of the micro ELISA plate well, avoid touching the inside wall and causing foaming as much as possible.</p>

	<p>2. Decant the solution from each well, add 350 μL of wash buffer to each well. Soak for 1 min and aspirate or decant the solution from each well and pat it dry against clean absorbent paper. Repeat this wash step 3 times. Note: a microplate washer can be used in this step and other wash steps. Make the tested strips in use immediately after the wash step. Do not allow wells to be dry.</p> <p>3. Add 100 μL of HRP Conjugate working solution to each well. Cover the plate with a new sealer. Incubate for 30 min at 37°C.</p> <p>4. Decant the solution from each well, repeat the wash process for 5 times as conducted in step 2.</p> <p>5. Add 90 μL of Substrate Reagent to each well. Cover the plate with a new sealer. Incubate for about 15 min at 37°C. Protect the plate from light. Note: the reaction time can be shortened or extended according to the actual color change, but not more than 30 min. Preheat the Microplate Reader for about 15 min before OD measurement.</p> <p>6. Add 50 μL of Stop Solution to each well. Note: adding the stop solution should be done in the same order as the substrate solution.</p> <p>7. Determine the optical density (OD value) of each well at once with a micro-plate reader set to 450 nm.</p>
Calculation of results	<p>Average the duplicate readings for each standard and samples. Plot a four parameter logistic curve on log-log axis, with standard concentration on the x-axis and OD values on the y-axis. If the OD of the sample under the lowest limit of the standard curve, you should re-test it with an appropriate dilution. The actual concentration is the calculated concentration multiplied by the dilution factor.</p>
Storage Stability	2-8°C
Typical data	<p>As the OD values of the standard curve may vary according to the conditions of the actual assay performance (e.g. operator, pipetting technique, washing technique or temperature effects), the operator should establish a standard curve for each test. Typical standard curve and data is provided below for reference only.</p>

	<table border="1"> <thead> <tr> <th>ng/mL</th> <th>OD</th> <th>Standard Curve</th> </tr> </thead> <tbody> <tr> <td>100</td> <td>0.418</td> <td rowspan="8">  </td> </tr> <tr> <td>50</td> <td>0.526</td> </tr> <tr> <td>25</td> <td>0.716</td> </tr> <tr> <td>12.5</td> <td>1.007</td> </tr> <tr> <td>6.25</td> <td>1.368</td> </tr> <tr> <td>3.13</td> <td>1.712</td> </tr> <tr> <td>1.56</td> <td>1.971</td> </tr> <tr> <td>0</td> <td>2.302</td> </tr> </tbody> </table>	ng/mL	OD	Standard Curve	100	0.418		50	0.526	25	0.716	12.5	1.007	6.25	1.368	3.13	1.712	1.56	1.971	0	2.302																					
ng/mL	OD	Standard Curve																																								
100	0.418																																									
50	0.526																																									
25	0.716																																									
12.5	1.007																																									
6.25	1.368																																									
3.13	1.712																																									
1.56	1.971																																									
0	2.302																																									
Precision	<p>Intra-assay Precision (Precision within an assay): 3 samples with low, mid range and high level HIS were tested 20 times on one plate, respectively. Inter-assay Precision (Precision between assays): 3 samples with low, mid range and high level HIS were tested on 3 different plates, 20 replicates in each plate, respectively.</p> <table border="1"> <thead> <tr> <th rowspan="2">Sample</th> <th colspan="3">Intra-assay Precision</th> <th colspan="3">Inter-assay Precision</th> </tr> <tr> <th>1</th> <th>2</th> <th>3</th> <th>1</th> <th>2</th> <th>3</th> </tr> </thead> <tbody> <tr> <td>n</td> <td>20</td> <td>20</td> <td>20</td> <td>20</td> <td>20</td> <td>20</td> </tr> <tr> <td>Mean</td> <td>5.17</td> <td>13.32</td> <td>45.10</td> <td>5.30</td> <td>13.54</td> <td>42.52</td> </tr> <tr> <td>Standard deviation</td> <td>0.27</td> <td>0.72</td> <td>1.51</td> <td>0.28</td> <td>0.61</td> <td>1.68</td> </tr> <tr> <td>C V (%)</td> <td>5.22</td> <td>5.41</td> <td>3.35</td> <td>5.28</td> <td>4.51</td> <td>3.95</td> </tr> </tbody> </table>	Sample	Intra-assay Precision			Inter-assay Precision			1	2	3	1	2	3	n	20	20	20	20	20	20	Mean	5.17	13.32	45.10	5.30	13.54	42.52	Standard deviation	0.27	0.72	1.51	0.28	0.61	1.68	C V (%)	5.22	5.41	3.35	5.28	4.51	3.95
Sample	Intra-assay Precision			Inter-assay Precision																																						
	1	2	3	1	2	3																																				
n	20	20	20	20	20	20																																				
Mean	5.17	13.32	45.10	5.30	13.54	42.52																																				
Standard deviation	0.27	0.72	1.51	0.28	0.61	1.68																																				
C V (%)	5.22	5.41	3.35	5.28	4.51	3.95																																				
Recovery	<p>The recovery of HIS spiked at three different levels in samples throughout the range of the assay was evaluated in various matrices.</p> <table border="1"> <thead> <tr> <th>Sample Type</th> <th>Range (%)</th> <th>Average Recovery (%)</th> </tr> </thead> <tbody> <tr> <td>Serum (n=8)</td> <td>90-100</td> <td>95</td> </tr> <tr> <td>EDTA plasma (n=8)</td> <td>87-100</td> <td>93</td> </tr> <tr> <td>Cell culture media (n=8)</td> <td>89-105</td> <td>97</td> </tr> </tbody> </table>	Sample Type	Range (%)	Average Recovery (%)	Serum (n=8)	90-100	95	EDTA plasma (n=8)	87-100	93	Cell culture media (n=8)	89-105	97																													
Sample Type	Range (%)	Average Recovery (%)																																								
Serum (n=8)	90-100	95																																								
EDTA plasma (n=8)	87-100	93																																								
Cell culture media (n=8)	89-105	97																																								
Linearity	<p>Samples were spiked with high concentrations of HIS and diluted with Reference Standard & Sample Diluent to produce samples with values within the range of the assay.</p> <table border="1"> <thead> <tr> <th></th> <th></th> <th>Serum (n=5)</th> <th>EDTA plasma(n=5)</th> <th>Cell culture media(n=5)</th> </tr> </thead> <tbody> <tr> <td rowspan="2">1:2</td> <td>Range (%)</td> <td>88-102</td> <td>88-103</td> <td>88-100</td> </tr> <tr> <td>Average (%)</td> <td>95</td> <td>95</td> <td>94</td> </tr> <tr> <td rowspan="2">1:4</td> <td>Range (%)</td> <td>85-98</td> <td>86-101</td> <td>87-99</td> </tr> <tr> <td>Average (%)</td> <td>91</td> <td>92</td> <td>94</td> </tr> <tr> <td rowspan="2">1:8</td> <td>Range (%)</td> <td>87-98</td> <td>89-100</td> <td>87-99</td> </tr> <tr> <td>Average (%)</td> <td>93</td> <td>95</td> <td>92</td> </tr> <tr> <td rowspan="2">1:16</td> <td>Range (%)</td> <td>86-99</td> <td>90-104</td> <td>89-102</td> </tr> <tr> <td>Average (%)</td> <td>92</td> <td>97</td> <td>96</td> </tr> </tbody> </table>			Serum (n=5)	EDTA plasma(n=5)	Cell culture media(n=5)	1:2	Range (%)	88-102	88-103	88-100	Average (%)	95	95	94	1:4	Range (%)	85-98	86-101	87-99	Average (%)	91	92	94	1:8	Range (%)	87-98	89-100	87-99	Average (%)	93	95	92	1:16	Range (%)	86-99	90-104	89-102	Average (%)	92	97	96
		Serum (n=5)	EDTA plasma(n=5)	Cell culture media(n=5)																																						
1:2	Range (%)	88-102	88-103	88-100																																						
	Average (%)	95	95	94																																						
1:4	Range (%)	85-98	86-101	87-99																																						
	Average (%)	91	92	94																																						
1:8	Range (%)	87-98	89-100	87-99																																						
	Average (%)	93	95	92																																						
1:16	Range (%)	86-99	90-104	89-102																																						
	Average (%)	92	97	96																																						
Kit components & Storage	<p>An unopened kit can be stored at 2-8°C for 1 month. If the kit is not supposed to be used within 1 month, store the items separately according to the following conditions once the kit is received.</p>																																									

Item	Specifications	Storage
Micro ELISA Plate (Dismountable)	96T: 8 wells ×12 strips 48T: 8 wells ×6 strips 24T: 8 wells ×3 strips 96T*5: 5 plates, 96T	-20°C, 6 months
Reference Standard	96T: 2 vials 48T/24T: 1 vial 96T*5: 10 vials	
Concentrated Biotinylated Detection Ab (100×)	96T: 1 vial, 120 µL 48T/24T: 1 vial, 60 µL 96T*5: 5 vials, 120 µL	
Concentrated HRP Conjugate (100×)	96T: 1 vial, 120 µL 48T/24T: 1 vial, 60 µL 96T*5: 5 vials, 120 µL	-20°C(shading light), 6 months
Reference Standard & Sample Diluent	96T/48T/24T: 1 vial, 20 mL 96T*5: 5 vials, 20 mL	2-8°C, 6 months
Biotinylated Detection Ab Diluent	96T/48T/24T: 1 vial, 14 mL 96T*5: 5 vials, 14 mL	
HRP Conjugate Diluent	96T/48T/24T: 1 vial, 14 mL 96T*5: 5 vials, 14 mL	
Concentrated Wash Buffer (25×)	96T/48T/24T: 1 vial, 30 mL 96T*5: 5 vials, 30 mL	
Substrate Reagent	96T/48T/24T: 1 vial, 10 mL 96T*5: 5 vials, 10 mL	2-8°C(shading light)
Stop Solution	96T/48T/24T: 1 vial, 10 mL 96T*5: 5 vials, 10 mL	2-8°C
Plate Sealer	96T/48T/24T: 5 pieces 96T*5: 25 pieces	
Product Description	1 copy	
Certificate of Analysis	1 copy	

Note: All reagent bottle caps must be tightened to prevent evaporation and microbial pollution.
The volume of reagents in partial shipments is a little more than the volume marked on the label, please use accurate measuring equipment instead of directly pouring into the vial(s).

Troubleshooting

Problem	Causes	Solutions
Poor standard curve	Inaccurate pipetting	Check pipettes.
	Improper standard dilution	Ensure briefly spin the vial of standard and dissolve the powder thoroughly by gentle mixing.
	Wells are not completely aspirated	Completely aspirate wells in between steps.
Low signal	Insufficient incubation time	Ensure sufficient incubation time.
	Incorrect assay temperature	Use recommended incubation temperature. Bring substrate to room temperature before use.
	Inadequate reagent volumes	Check pipettes and ensure correct preparation.
	Improper dilution	
	HRP conjugate inactive or TMB failure	Mix HRP conjugate and TMB, rapid coloring.
Deep color but low value	Plate reader setting is not optimal	Verify the wavelength and filter setting on the Microplate reader.
		Open the Microplate Reader ahead to pre-heat.
Large CV	Inaccurate pipetting	Check pipettes.
High background	Concentration of target protein is too high	Use recommended dilution factor.
	Plate is insufficiently washed	Review the manual for proper wash. If using a plate washer, check that all ports are unobstructed.
	Contaminated wash buffer	Prepare fresh wash buffer.
Low sensitivity	Improper storage of the ELISA kit	All the reagents should be stored according to the instructions.
	Stop solution is not added	Stop solution should be added to each well before measurement.